

# DERMAGRIP®

## Examination Gloves


Powder Free Latex Examination Gloves

DERMAGRIP Powder Free

DERMAGRIP Classic Powder Free

DERMAGRIP Powder Free, Sterile

DERMAGRIP Polymer Coated Powder Free

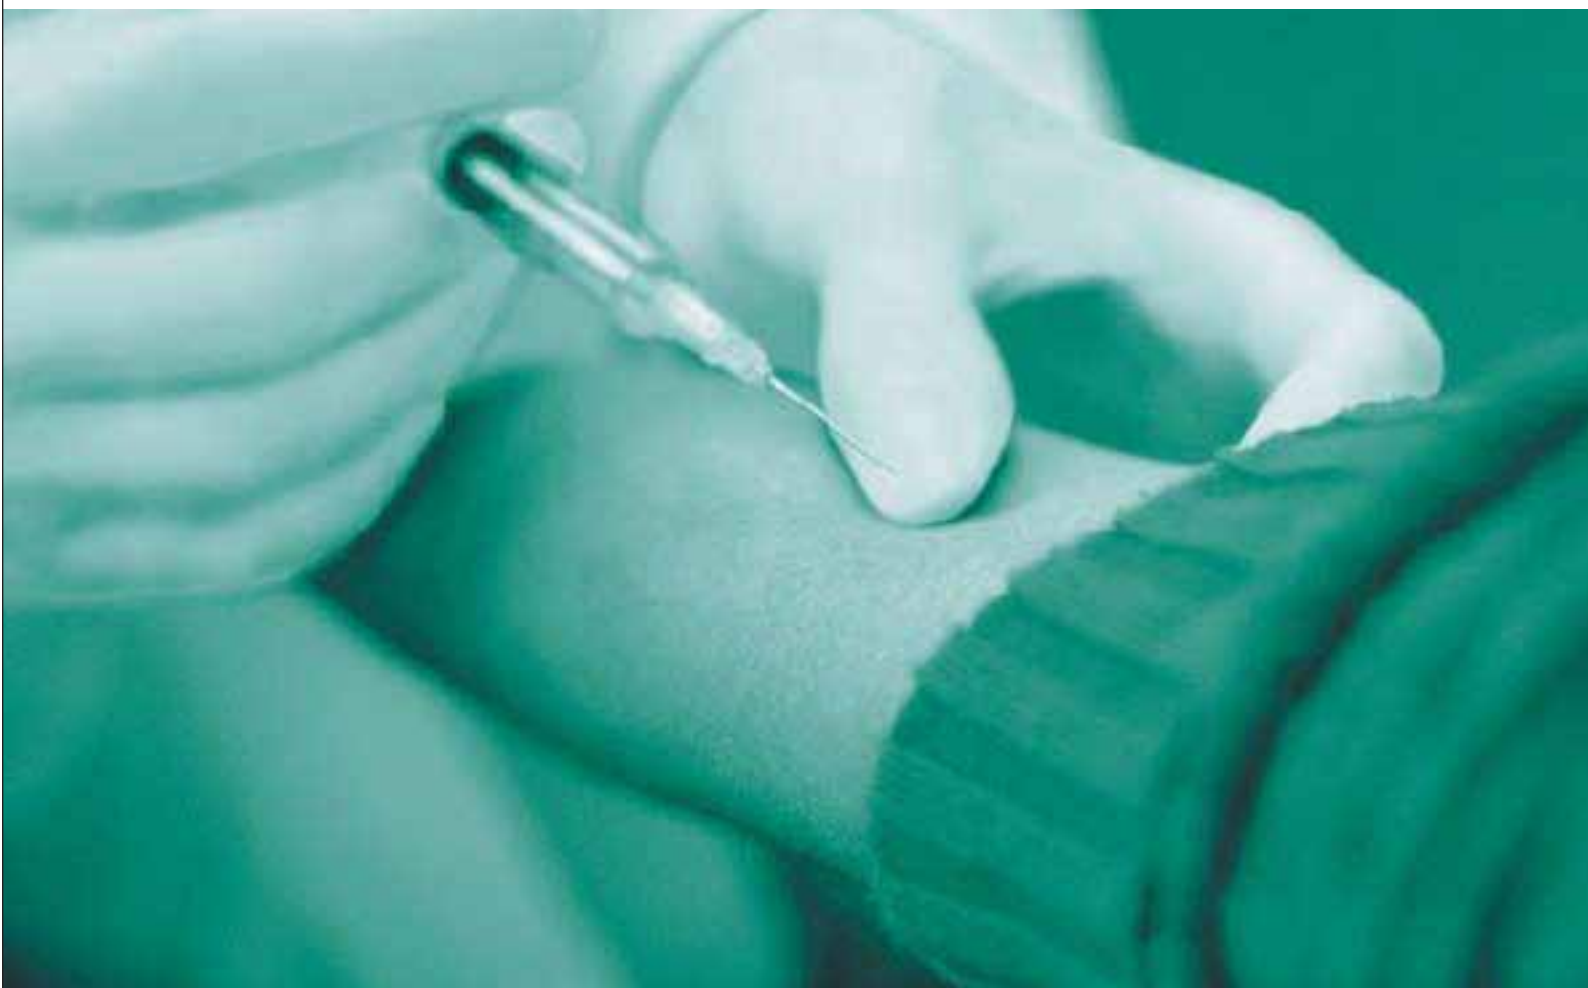

Natural Rubber Latex

Powder Free

Low Protein

Unique Surface Texture



Your Partner In Protection™

## Examination Gloves

### Exceptional Performance

Medical gloves serve to provide protection from unwanted and dangerous substances for both healthcare professionals and their patients. **DERMAGRIP® Examination Gloves** are designed to meet and exceed international product standards using sophisticated technologies and innovations to provide uncompromized protection to its users.

**DERMAGRIP® Examination Gloves** stand out for its unique surface texture allowing for extra sensitivity. This is the preferred glove whenever extra sensitivity and special surface texture is important.

• Powder free feature eliminates powder-induced irritation and powder stains

• Textured surface for enhanced grip



• Minimum level of NR latex proteins and undetectable chemical residues greatly reduce allergic skin reactions

• High tensile strength minimizes tear

• Excellent fit and feel

• Beaded cuff for easy donning




BSI PS (0086), HP2 45Q, UK



BS EN 374-2:2003  
Micro-organism  
Hazards



GKL  
BS EN 374-3:2003  
Chemical Hazards



BS EN 388:2003  
Mechanical  
Hazards

### PRODUCT INFORMATION

**Type:** Powder free and non-sterile

**Primary Material:** Natural rubber latex

#### Dimensions:

Glove Size	Reorder#	Palm Width (mm)	Length (mm)
Extra-small	D1500-30	≤ 80	240 min
Small	D1501-30	80 ± 10	240 min
Medium	D1502-30	95 ± 10	240 min
Large	D1503-30	110 ± 10	240 min
Extra-large	D1504-30	≥ 110	240 min

#### Thickness:

Location of Thickness Measurements	Single Wall (mm)
Finger (at 15 mm from the extreme tip)	0.16 ± 0.03
Palm (at center of palm)	0.14 ± 0.03
Cuff (at 25 mm from cuff end)	0.11 ± 0.03

#### Physical Properties:

Parameters	Before Aging	After Aging
Tensile Strength (MPa)	≥ 21	≥ 18
Force At Break (N)	≥ 9	≥ 6

**Powder:** No powder lubricant added. Light chlorinated on glove surface

**Protein Content:** This latex glove contains 50 micrograms or less of total water extractable protein per gram of glove

**Color:** Off white to yellow

**Design and Feature:** Ambidextrous, textured surface overall and beaded cuff

**Packing:** 100 gloves per dispenser, 10 dispensers per carton

#### Pre-shipment Quality Inspection:

Criteria	Insp. Level	AQL
Dimension	N=13	Median
Physical Properties	N=13	Median
1000ml Water Leak Test	G-I	1.5
Visual Inspection for Major Defects	G-I	2.5
Visual Inspection for Minor Defects	G-I	4.0
Powder Free Residue	N=5	N/A
Protein Contant	N=8	N/A

#### Product Conformance:

- Medical Device: in compliance with European Medical Device Directive 93/42/EEC (CE Class I).
- Personal Protective Equipment of Complex Design Category III, in compliance with 89/686/EEC, type tested to EN 420:2003+A1:2009, EN 374-2:2003, EN 374-3:2003 & EN 388:2003, CE 0086.
- ASTM D3578.

**Quality Assurance:** Manufacturing process is in compliance with US FDA Quality System Regulation (QSR) and ISO9001 and ISO13485 Quality Systems



**WRP Asia Pacific Sdn Bhd** 1 4 7 8 1 7 V

Lot 1, Jalan 3, Kawasan Perusahaan  
Bandar Baru Salak Tinggi,  
43900 Sepang, Selangor Darul Ehsan,  
MALAYSIA

Office +60-3-8706 1486

Facsimile +60-3-8706 1557

Email customer\_wrp@wrpworld.com



**REMESCO Handelges.m.b.H.**

Grinzinger Allee 5/25, 1190 Vienna,  
AUSTRIA

Office +43-1-328-50-88

Facsimile +43-1-328 29-49

Email office@remesco.com

Distributed by: